



### Air and Emissions Fibers

**Shipment:** 404      **Matrix:** Air and Emissions  
**Analyte:** Fibers  
**Sample:** 1090  
**Technology:** PCM  
**Prep Method:**  
**Target:** 232.64      Fibers per mm2  
**Limits:** 67.6 to 354 Fibers per mm2  
**Basis:** Robust Statistics (Normal Distribution)  
**Robust Mean:** 210.8 Fibers per mm2  
**Std Dev:** 57.334 Fibers per mm2  
**Median:** 209.135 Fibers per mm2  
**Totals for Matrix/Analyte/Technology:**  
**Labs: Pass:** 84      **Fail:** 2      **Total:** 86  
**Totals for Matrix/Analyte:**      **Labs: Pass:** 84      **Fail:** 2      **Total:** 86

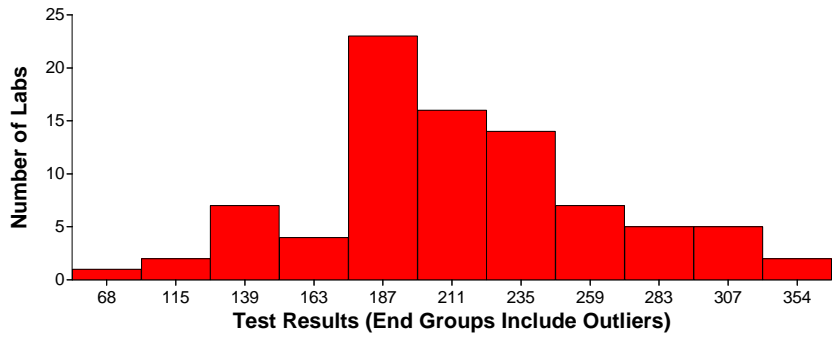


### Air and Emissions Fibers

**Shipment:** 404      **Matrix:** Air and Emissions  
**Analyte:** Fibers  
**Sample:** 6061  
**Technology:** PCM  
**Prep Method:**  
**Target:** 90.18      Fibers per mm2  
**Limits:** 17.5 to 137 Fibers per mm2  
**Basis:** Robust Statistics (Normal Distribution)  
**Robust Mean:** 77.4 Fibers per mm2  
**Std Dev:** 23.5649 Fibers per mm2  
**Median:** 78.95 Fibers per mm2  
**Totals for Matrix/Analyte/Technology:**  
**Labs: Pass:** 84      **Fail:** 2      **Total:** 86  
**Totals for Matrix/Analyte:**      **Labs: Pass:** 84      **Fail:** 2      **Total:** 86

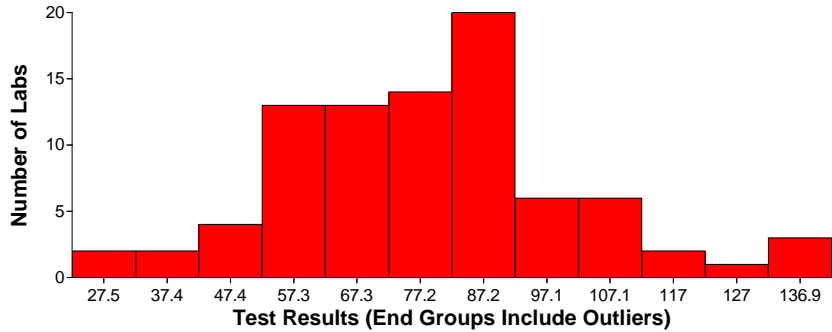


### Air and Emissions Fibers

**Shipment:** 404      **Matrix:** Air and Emissions  
**Analyte:** Fibers  
**Sample:** 6650  
**Technology:** PCM  
**Prep Method:**  
**Target:** 588.42      Fibers per mm2  
**Limits:** 90 to 864 Fibers per mm2  
**Basis:** Robust Statistics (Normal Distribution)  
**Robust Mean:** 478.8 Fibers per mm2  
**Std Dev:** 147.9129 Fibers per mm2  
**Median:** 475 Fibers per mm2  
**Totals for Matrix/Analyte/Technology:**  
**Labs: Pass:** 84      **Fail:** 2      **Total:** 86  
**Totals for Matrix/Analyte:**      **Labs: Pass:** 84      **Fail:** 2      **Total:** 86

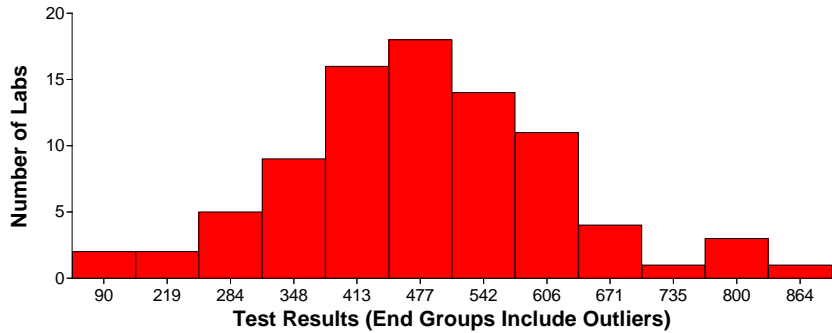

### Air and Emissions Fibers

**Shipment:** 404      **Matrix:** Air and Emissions  
**Analyte:** Fibers  
**Sample:** 7516  
**Technology:** PCM  
**Prep Method:**  
**Target:** 172.14      Fibers per mm2  
**Limits:** 35.5 to 249 Fibers per mm2  
**Basis:** Robust Statistics (Normal Distribution)  
**Robust Mean:** 142.1 Fibers per mm2  
**Std Dev:** 42.0997 Fibers per mm2  
**Median:** 142.15 Fibers per mm2  
**Totals for Matrix/Analyte/Technology:**  
**Labs: Pass:** 83      **Fail:** 3      **Total:** 86  
**Totals for Matrix/Analyte:**      **Labs: Pass:** 83      **Fail:** 3      **Total:** 86

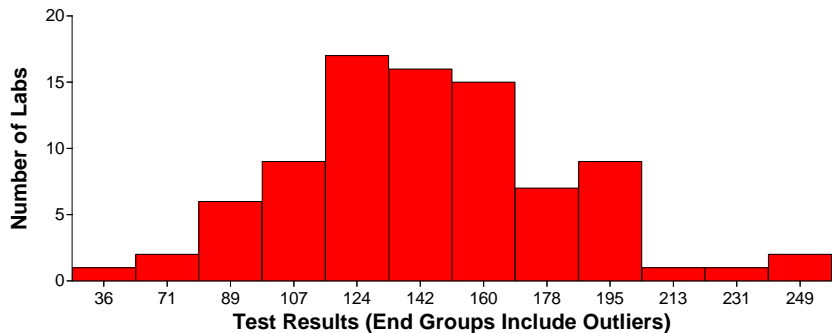

### Solid and Hazardous Waste Asbestos in Friable Material

### Solid and Hazardous Waste Asbestos in Friable Material

Shipment: 404 Matrix: Solid and Hazardous Waste

Analyte: Asbestos in Friable Material

Sample: 6309

Technology: PLM

Prep Method:

Target: 10.7 %

Limits: 1 to 12 %

Basis: Swa scoring

Robust Mean: 3.7 %

Std Dev: 1.8274 %


Median: 3.5 %

Totals for Matrix/Analyte/Technology:

Labs: Pass: 71 Fail: 2 Total: 73

Totals for Matrix/Analyte: Labs: Pass: 71 Fail: 2 Total: 73

---

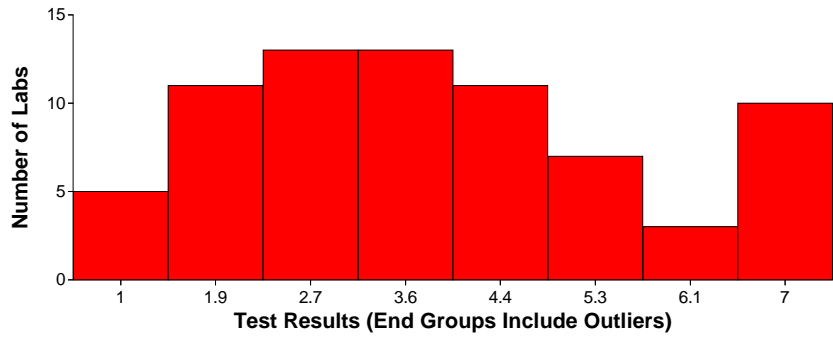

### Solid and Hazardous Waste Asbestos in Friable Material

Shipment: 404 Matrix: Solid and Hazardous Waste

Analyte: Asbestos in Friable Material

Sample: 9993

Technology: PLM

Prep Method:

Target: 5 %

Limits: 1 to 6.5 %

Basis: Swa scoring

Robust Mean: 3.3 %

Std Dev: 1.7935 %

Median: 3 %

Totals for Matrix/Analyte/Technology:

Labs: Pass: 66 Fail: 7 Total: 73

Totals for Matrix/Analyte: Labs: Pass: 66 Fail: 7 Total: 73

---

